Ewen-Parker X-Ray Corporation

Automatic Processor Quality Control Chart

Facility:_____ **Month / Year:**_____

Date	1	2	3	4	5	6	7	8	9	10	11	12	13	14	15	16	17	18	19	20	21	22	23	24	25	26	27	28	29	30	31
Dev. Temp																															
✓Crossover																															
✓P.M.																															

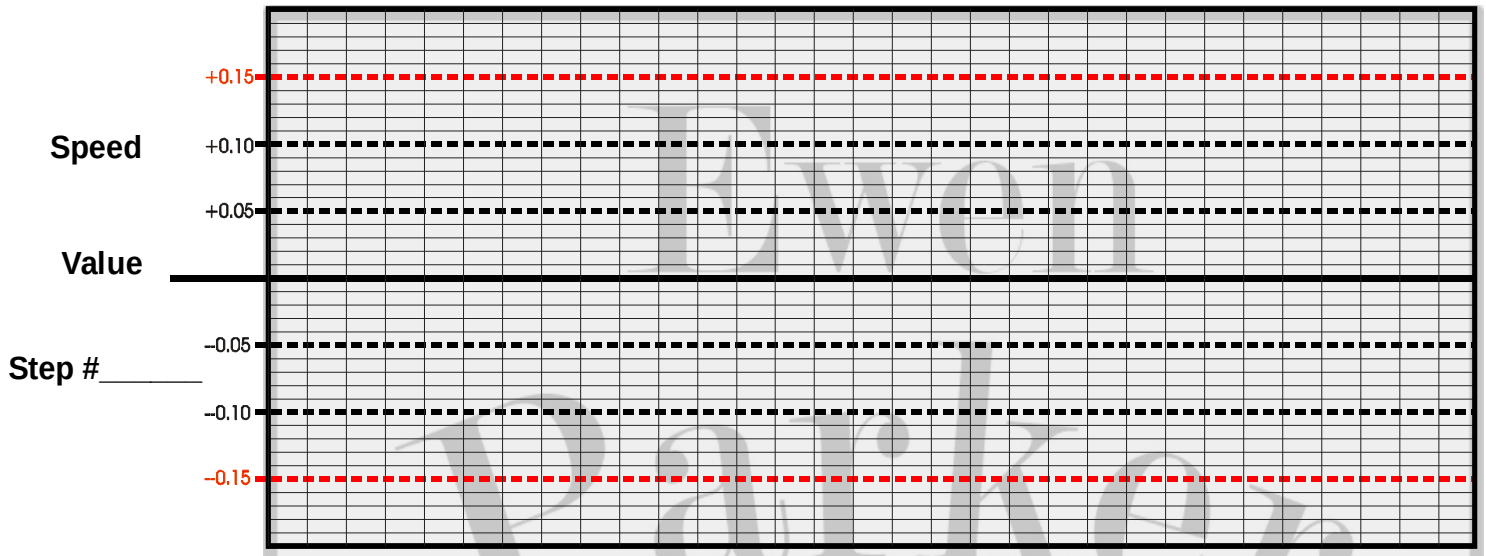

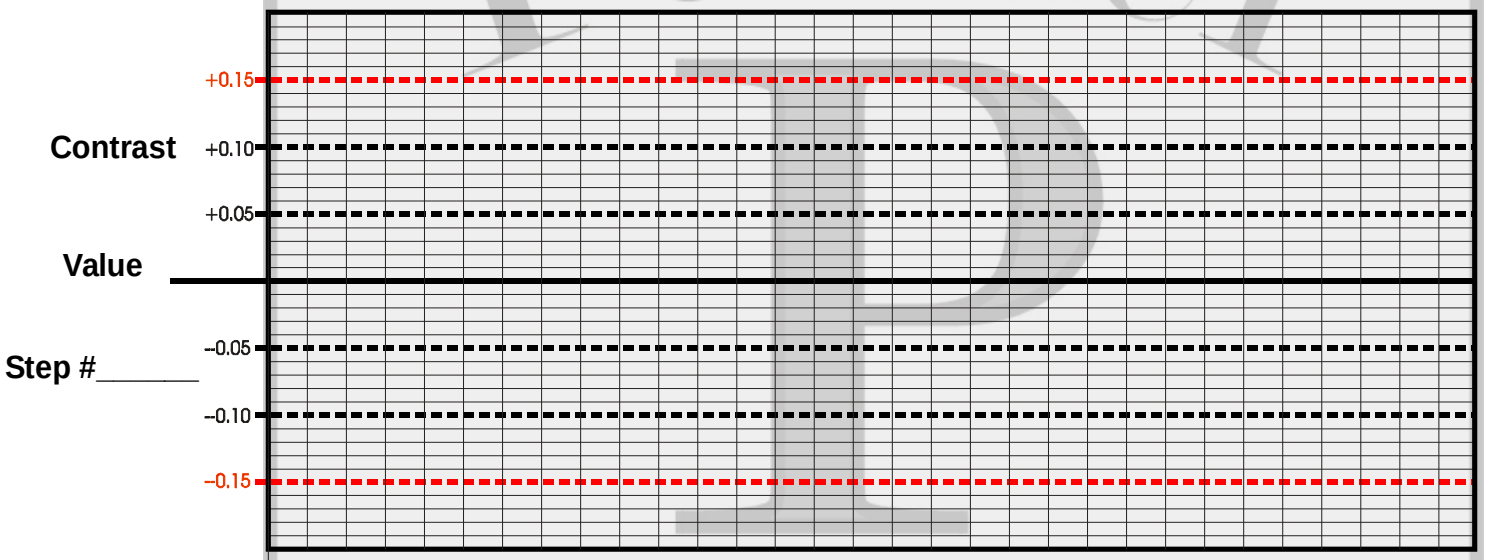

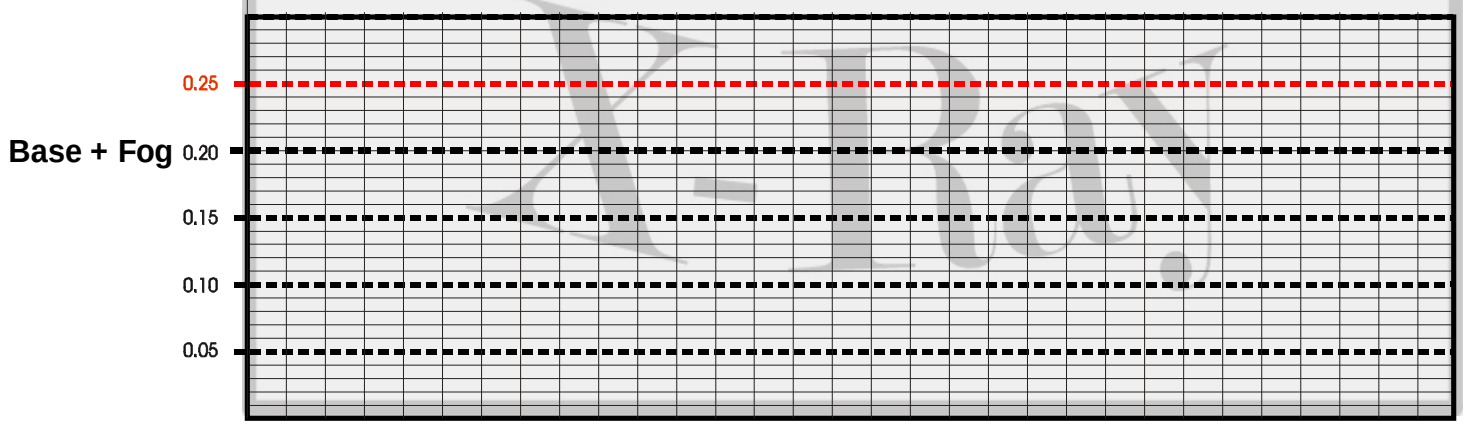

Ewen Parker X-Ray